


## Scanning electron micrographs of *M. mycoides* JCVI-syn1.0

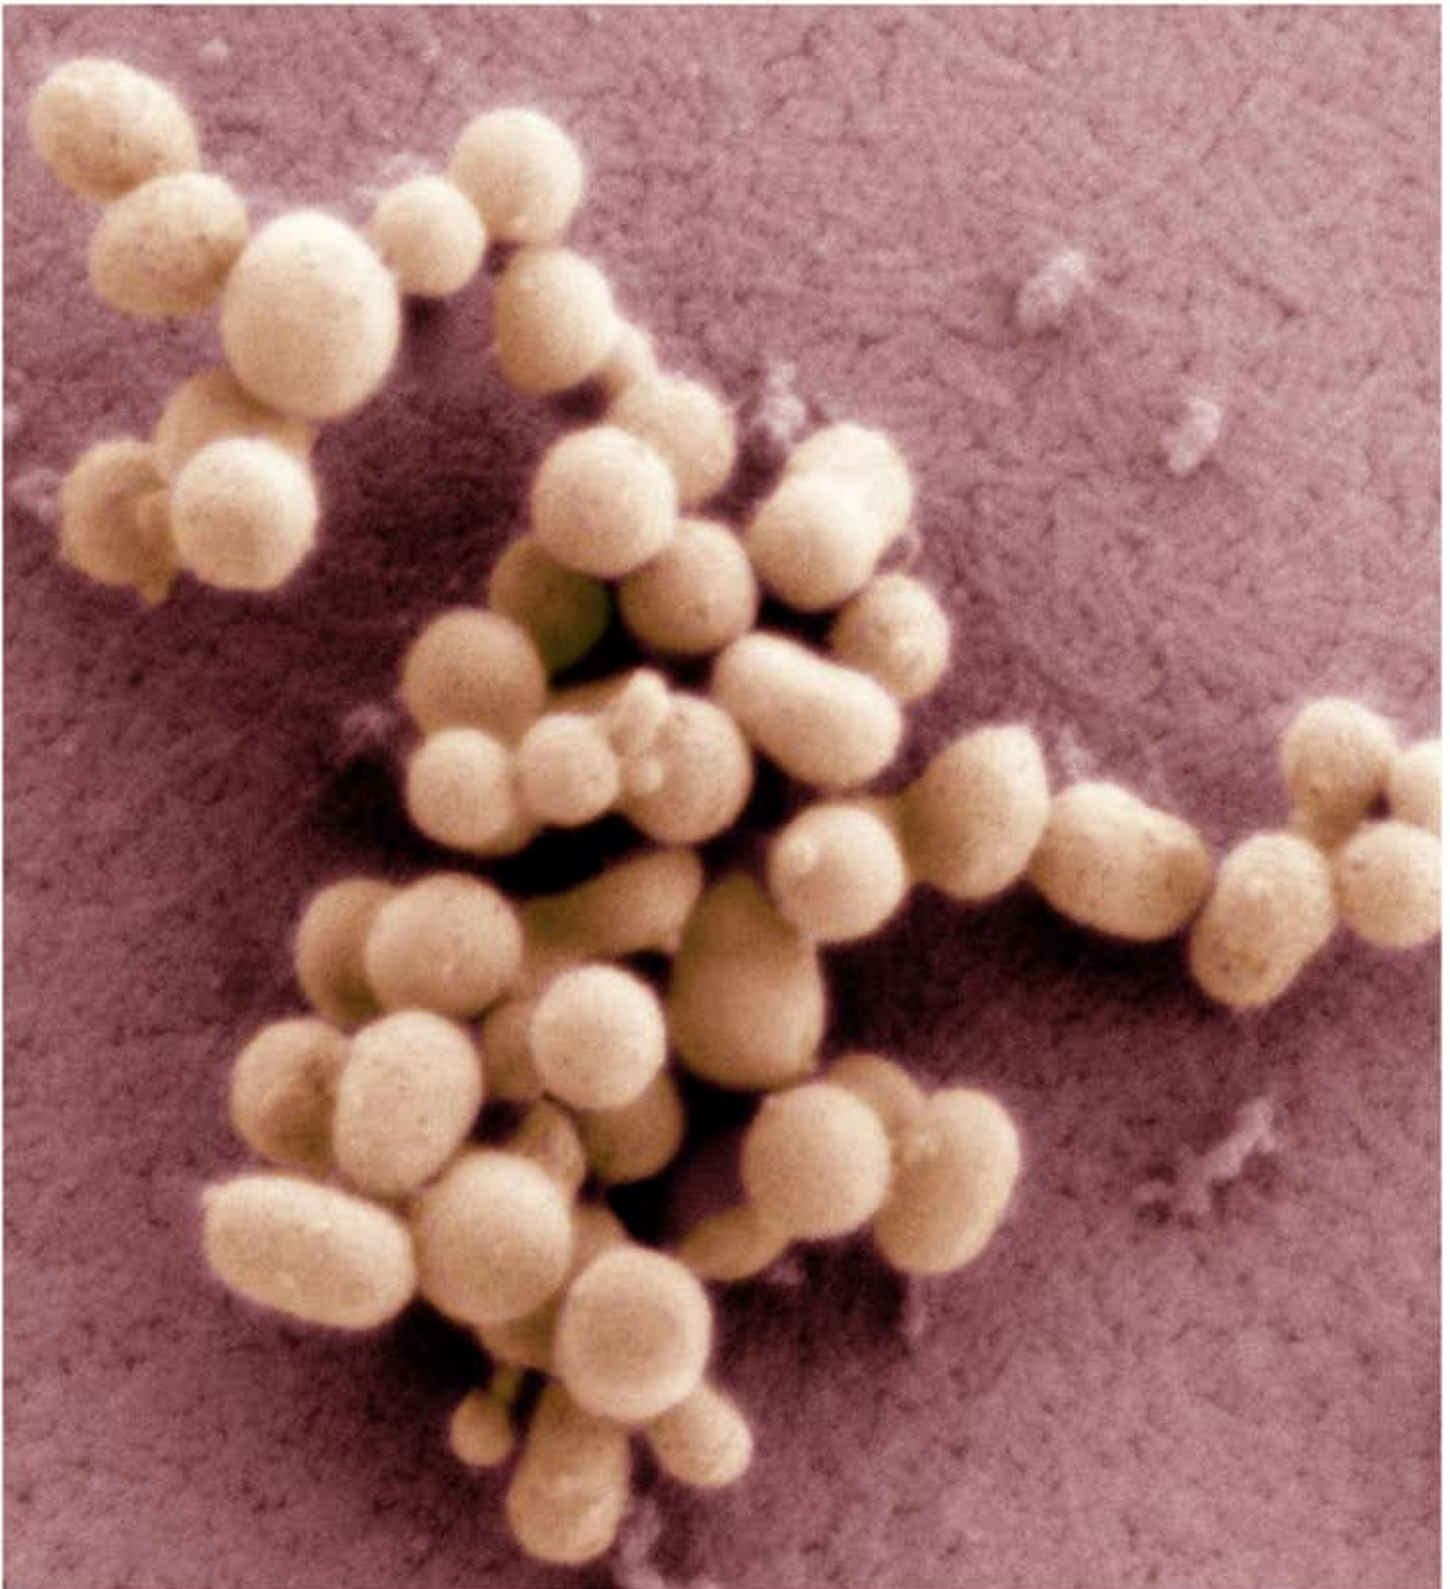

Samples were post-fixed in osmium tetroxide, dehydrated and critical point dried with CO<sub>2</sub>, then visualized using a Hitachi SU6600 scanning electron microscope at 2.0 keV. Electron micrographs were provided by Tom Deerinck and Mark Ellisman of the National Center for Microscopy and Imaging Research at the University of California at San Diego.